

WIDEX MENU™

THE CHOICE IS YOURS

USER INSTRUCTIONS  
**THE MENU™ SERIES**

ME-*m* model  
Behind-the-ear

# YOUR WIDEX HEARING AID

*(To be filled out by the hearing care professional)*

- ME3-*m*
- ME5-*m*
- ME10-*m*

Date: \_\_\_\_\_

Battery size: 10

Programs:

<input checked="" type="checkbox"/> Master
<input type="checkbox"/> Music
<input type="checkbox"/> TV
<input type="checkbox"/> Standard
<input type="checkbox"/> Acclimatization
<input type="checkbox"/> Audibility Extender
<input type="checkbox"/> ZEN

# CONTENTS

<b>SYMBOLS</b> .....	<b>4</b>
<b>DESCRIPTION OF THE HEARING AID</b> .....	<b>5</b>
Right/left identification .....	8
Acoustic indicators .....	8
The battery.....	9
Inserting the battery.....	9
Removing the battery.....	11
Battery drawer without a nail grip .....	12
Low battery indication .....	13
Turning the hearing aid on and off.....	14
Positioning the hearing aid .....	15
Removing the hearing aid .....	16
Volume adjustment.....	17
Listening programs.....	18
Switching between the listening programs .....	23
Using a telephone .....	24
<b>CLEANING</b> .....	<b>25</b>
The hearing aid .....	26
The microphone openings .....	26
<b>ACCESSORIES</b> .....	<b>27</b>
<b>IN CASE OF MALFUNCTION</b> .....	<b>28</b>
<b>CARING FOR YOUR HEARING AID</b> .....	<b>29</b>
<b>WARNINGS</b> .....	<b>30</b>
<b>ADVICE</b> .....	<b>33</b>
<b>REGULATORY INFORMATION</b> .....	<b>34</b>

# SYMBOLS

The following symbols will be used throughout the manual:



Messages with this heading indicate serious adverse reactions, potential safety hazards and inadequate performance of device.



Messages with this heading indicate/include information regarding any special care to be exercised.




 Not for general waste.

## DESCRIPTION OF THE HEARING AID

Your hearing aid is used with an ear-set which consists of a tube and an ear-tip or earmold.

The illustration below shows the hearing aid without an ear-set. The choice of ear-set solution depends on your specific needs. Please refer to the separate ear-set user manual.

- 1. Microphone openings**
- 2. Program button** (*available in some versions*)
- 3. On/off function** (*integrated into the battery drawer*)
- 4. Nail grip**
- 5. RL ID**

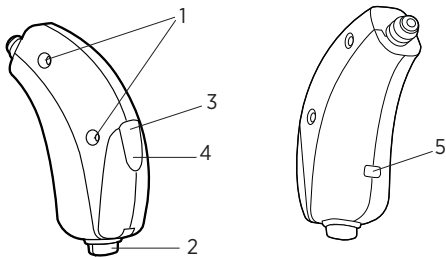

Your hearing aid may be provided with an optional listening program called Zen. It makes musical tones (and sometimes a rushing noise) in the background. These sounds are shaped according to your hearing loss.

## NOTE

In addition to these user instructions, a separate user manual is provided describing the various ear-set solutions available for your hearing aid: “Ear-sets for Widex BTE hearing aids”.



### **WARNING**

This booklet and the manual “Ear-sets for Widex BTE hearing aids” contain important information and instructions. Read these booklets carefully before you start using the hearing aid.

## NOTE

Your hearing aid, ear-set and accessories may not look exactly as illustrated in this booklet. We also reserve the right to make any changes considered necessary.

### **Intended use**


The hearing aids are intended as air conduction amplification devices to be used in everyday listening environments. The hearing aids may be provided with the Zen program intended to provide a relaxing sound background (i.e. music/noise source) for adults who desire to listen to such a background in quiet.

### **Indications for use**

The devices are indicated for individuals with a range of hearing loss severity from minimal (10 dB HL) to severe (80 dB HL) and all hearing loss configurations.

They are to be programmed by licensed hearing care professionals (audiologists, hearing aid specialists, otolaryngologists) who are trained in hearing (re)habilitation as well as tinnitus management.

## Right/left identification



If you wear hearing aids on both ears, the hearing aids can be provided with colored marks (red mark = right and blue mark = left).

The arrow shows the position of the identification mark.

## Acoustic indicators

The hearing aid may be set to produce a signal to indicate the use of certain functions. The signal may be tones (SmartTone) or a spoken message (SmartSpeak)\*. The signal can also be deactivated.

Functions	Default settings	Other settings
Adjusting volume via remote control	<b>Tone</b>	Off
Confirming program button use	<b>Clicking sound</b>	Off
Changing program	<b>Tones</b>	Message/off
Starting up the hearing aid	<b>Tone</b>	Message/off
Warning about low battery	<b>4 tones</b>	Message/off
Service reminder	<b>Off</b>	Message

\* *SmartSpeak not available as a standard feature*



## The battery

We recommend **zinc-air batteries**. Use a **size 10** battery for the hearing aid.

To obtain replacement batteries, please consult your hearing care professional. It is important to take note of the expiration date and the recommendations on the battery pack regarding disposal of used batteries. Otherwise there is a risk that the battery life may be reduced.



### Inserting the battery


Before inserting a new battery into the hearing aid, remember to remove the adhesive tab. Once the tab has been removed, the battery will start functioning after a few seconds.




#### CAUTION

Do not use batteries if there is a sticky residue from the tab or other unwanted substance, as this can cause the hearing aid to malfunction.

Use the nail grip to gently swing the battery drawer open. Do not press the drawer beyond the open position.

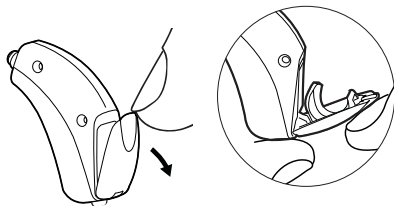

Place the battery in the drawer as illustrated, so that the plus (+) sign on the battery is facing towards you when you hold the hearing aid as shown. You can use the battery magnet provided to steer the battery into place.

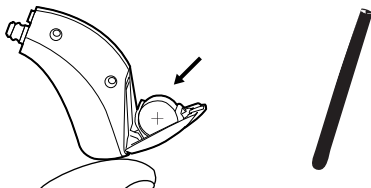


If the battery drawer does not close easily, the battery is incorrectly inserted.

When changing battery, it is a good idea to hold the hearing aid over a table.

## Removing the battery


1. Open the battery drawer as previously described. Place the hearing aid on the provided cloth on a clean, plane surface and turn it as illustrated.
2. Supporting the drawer with your finger, use the battery magnet provided to push the battery out of the battery drawer from the minus side.

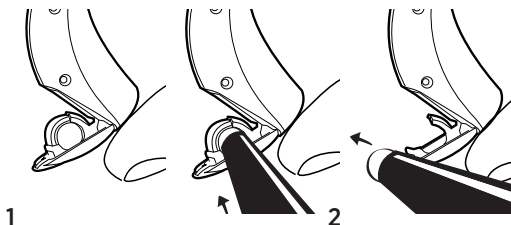

## Battery drawer without a nail grip



The hearing aid may be provided with a battery drawer without a nail grip, which means that you need a tool to open the battery drawer. This type of drawer can be a good choice if the hearing aid is worn by a child. A special tool for opening the drawer will be included with this drawer.

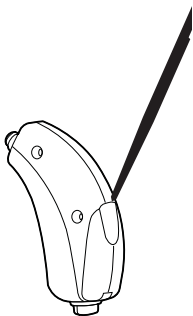

The battery drawer is opened as illustrated.

## Low battery indication

An acoustic indicator will sound when the battery is nearly exhausted, unless this function has been disabled (see page 8). We recommend that you always have a spare battery with you.



### WARNING

**Never** leave an exhausted battery in the hearing aid. Exhausted batteries may leak, damaging the hearing aid.




### WARNING


Your hearing aid may stop functioning, for instance if the battery is exhausted. You should be aware of this possibility, in particular when you are in traffic or are otherwise dependent on warning signals.

## Turning the hearing aid on and off

The battery drawer of the hearing aid also functions as the on/off switch.



Close the battery drawer to turn on the hearing aid. An acoustic indicator will indicate that the hearing aid has been switched on unless this function has been disabled.




Open the battery drawer completely to turn off the hearing aid.

Please remember to turn off the hearing aid when it is not in use. Remove the battery if the hearing aid will not be used for several days.

## Positioning the hearing aid

Insert the earpiece in the ear canal while holding the lower part of the tube. It may help to pull the outer ear backwards and upwards with the opposite hand.

Place the hearing aid behind the ear, so that the hearing aid and tube rest comfortably on the ear, close to your head.

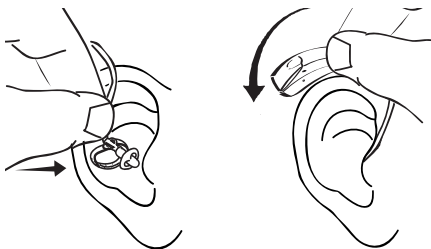

The illustrations show an open ear-tip. For further information on ear-tip/earmold types, anchors and procedures, see the separate ear-set user manual provided.

## Removing the hearing aid

Remove the hearing aid from its position behind the ear.

Carefully pull the earpiece out of the ear canal, while holding the lower part of the tube. If the earpiece is provided with an extraction cord, take hold of this and carefully pull the ear-tip out of the ear canal.





## Volume adjustment

The hearing aid volume is adjusted automatically in accordance with your sound environment.

If you have a remote control, you can also adjust the volume manually or mute your hearing aid. Any adjustment of the volume setting will be canceled when your hearing aid is turned off, or when you change program.

If you have a remote control, please also refer to the user instructions for this.



### CAUTION

If the volume in the hearing aid is generally too loud or too weak, or the reproduced sounds are distorted, or if you would like any further information, consult your hearing care professional.

### To mute the hearing aid with a remote control:

Keep pressing the volume down key on the remote control after the long beep-tone has sounded and until it stops. Pressing one of the volume keys briefly will bring back the sound.

## Listening programs

By default, your hearing aid contains a Master program. With a program button or remote control, you have the option of an extra program, and a number of supplementary programs can also be made available. If this solution is chosen, you can have up to five programs.

<b>Master</b>	All the automatic functions work to ensure comfort in all listening situations
<b>Music</b>	For listening to music
<b>TV</b>	For listening to the TV
<b>Standard</b>	All the automatic functions work to ensure audibility and speech understanding in all listening situations
<b>Acclimatization</b>	This program has the same features as the Master program but provides slightly less amplification
<b>Audibility Extender*</b>	Makes high-frequency sounds audible
<b>Zen*</b>	Generates different kinds of tones.

*\* Available separately*

If your needs change over time, the combination of listening programs can be altered.

## Zen program

Your hearing aid may be provided with a unique optional listening program called Zen. It makes musical tones (and sometimes a rushing noise) in the background. These sounds are shaped according to your hearing loss. The Zen program may be used alone (without amplification) in quiet when you are not required to hear surrounding sounds. Or, it may be used with the Master program so both the surrounding sounds and the generated sounds (fractal tones and noise) are heard together.



### CAUTION

Use of the different Zen programs may interfere with hearing surrounding sounds including speech. The programs should not be used when hearing such sounds is important. Switch the hearing aid to a non-Zen program in those situations.



### CAUTION

If you perceive a decrease in loudness, tolerance of sounds, speech not as clear, or worsening tinnitus, contact your hearing care professional.

## **Benefits**

The Zen program may provide a relaxing listening background for some people. When the Zen program is used in a tinnitus management program, its wearer may experience some relief from tinnitus.

## **Indications for use**

The Zen program is intended to provide a relaxing sound background (i.e., music/noise source) for adults who desire to listen to such a background in quiet. It may be used as a sound therapy tool in a tinnitus treatment program that is prescribed by a hearing care professional (audiologists, hearing aid specialists, otolaryngologists) who is trained in tinnitus management.

## **Directions for use**

Because of the unique ways in which Zen is programmed in your hearing aid, please follow the recommendations of your hearing care professionals as to how to use the program, when to use the program and/or how long to use the program.

## **Precautions**

To ensure the safety and effectiveness of the Zen program when used as a sound therapy tool for tinnitus, the tinnitus management program must be designed and conducted by hearing care professionals who are trained in tinnitus management. A tinnitus management program should include a complete audiological evaluation, tinnitus diagnosis, counseling, use of proper amplification and/or sound therapy tools.

Prior to any tinnitus management program, it is advisable that you seek medical attention to exhaust any medical or surgical treatment options.

Use your hearing aid and the Zen program according to the directions and schedule recommended by your hearing care professionals.


## **Warnings**

Use of the Zen program may interfere with hearing everyday sounds including speech. It should not be used when hearing such sounds is important. Switch the hearing aid to a non-Zen program in those situations.

## **Risks**

There are no known risks or side effects associated with the use of the Zen program. However, consistent with our recommendations on the use of conventional hearing aids, stop using the hearing aids (and the Zen program) and seek attention from your hearing care professional if any of the following symptoms are noted:

- Skin irritation
- Perceived decrease in loudness, tolerance of sounds, speech not as clear, or worsening tinnitus



## Switching between the listening programs

To change programs, press the program button (if available) on the hearing aid or the remote control program key briefly. Each time you change program an acoustic indicator will sound unless this function has been disabled.

**Program 1:** One short beep or message

**Program 2:** Two short beeps or message


---

**Program 3:** Three short beeps or message

**Program 4:** One long and one short beep or message

**Program 5:** One long and two short beeps or message

## Using a telephone




When using a telephone, we recommend that you hold the telephone against your head at an angle above your ear, rather than directly against the ear. If the sound is not optimal, try moving the telephone earpiece to a slightly different position.



# CLEANING

The following cleaning accessories are available for the hearing aid and ear-set \*. For cleaning the ear-set, see the user manual “Ear-sets for Widex BTE hearing aids”.

1. Cloth
2. Wax removing tool
3. Cleaning thread

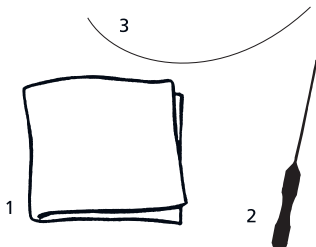

Contact your hearing care professional if you need additional supplies of cleaning accessories.

*\* Selection depends on ear-set type*




## The hearing aid

Clean the hearing aid with the soft cloth after use.



### WARNING


**Never** use water or cleaning solutions to clean the hearing aid, as this may cause it to malfunction.



## The microphone openings


Clean the microphone openings by passing the wax removing tool straight through the openings.

If you feel resistance, withdraw the tool and try again. Use only the wax removing tool provided.



When the hearing aid is not in use, the battery drawer should be left open, to ventilate the hearing aid and allow it to dry.

## ACCESSORIES



### Remote control

Some hearing aids of the model you have may be provided with a remote control. These hearing aids have no program button. If your hearing aid has a remote control, please also refer to the user instructions for this.

## IN CASE OF MALFUNCTION

Problem	Possible cause	Solution
The hearing aid is completely silent	The hearing aid is not turned on	Make sure the battery drawer is closed
	The battery does not work	Insert a new battery in the battery drawer
The hearing aid volume is not powerful enough	The battery is nearly exhausted	Insert a new battery in the battery drawer
	Your ear is blocked by earwax	Contact your ENT doctor/physician
	Your hearing may have changed	Contact your hearing care professional
The hearing aid whistles continuously	Your ear is blocked by earwax	Contact your ENT doctor/physician

**Note:** This information covers only the hearing aid. See the “Ear-sets for Widex BTE hearing aids” user manual for information specific to your ear-set.

If the problems persist, contact your hearing care professional for assistance.

## CARING FOR YOUR HEARING AID

The hearing aid is a valuable object and should be treated with care. Here are some things you can do to prolong the life of your hearing aid:



### CAUTION

- Turn off your hearing aid when it is not in use. Remove the battery if the hearing aid will not be used for several days.
- When the hearing aid is not in use, keep it in its case in a dry location out of reach of children and pets.
- Do not expose the hearing aid to extreme temperatures or high humidity. Make sure to dry the hearing aid thoroughly after heavy perspiration such as that which may occur during intense physical activity, e.g. playing sports.
- Avoid dropping your hearing aid – perform cleaning and battery changes while holding the hearing aid above a soft surface.
- Do not wear your hearing aid while in the shower or swimming, or when using a hair dryer, perfume, hair and body sprays or gels such as suntanning lotions or creams.
- In environments with high humidity, a drying kit may be used daily to reduce the amount of moisture inside the hearing aid. See the instructions enclosed with the drying kit.

## WARNINGS



### WARNING

Hearing aids and batteries can be dangerous if swallowed or used improperly. Swallowing or improper use can result in severe injury or even fatalities. In case of ingestion, contact a physician immediately and the 24 Hour National Button Battery Ingestion Hotline at (202) 625-3333.

- Keep hearing aids and their parts, accessories and batteries out of reach of children and anyone else who might swallow such items or otherwise cause injury to themselves. Do not change batteries in front of them and do not let them see where you keep your battery supply. Discard used batteries carefully.
- Batteries are very small and can easily be mistaken for pills or the like. Never put a battery or hearing aid in your mouth for any reason as you may risk swallowing it.



## WARNING

- Risk of explosion if battery is replaced by an incorrect type or recharged. Dispose of used batteries according to the instructions.
- Never allow others to wear your hearing aid, as this could cause permanent damage to their hearing.
- When selecting a listening program, please remember that there are situations in which it is particularly important to be able to hear the surrounding sounds (e.g. traffic, warning signals).
- The hearing aid is made of modern non-allergenic materials. Nonetheless, in rare cases skin irritation may occur. If you notice skin irritation in or around your ear or ear canal, contact your hearing care professional.



## WARNING

- Be aware that the use of any type of hearing aid may involve a slightly increased risk of infection in the ear canal. An infection can arise as a result of inadequate ventilation of the ear. We therefore recommend that you remove the hearing aid and ear-set from your ear at night to allow the ear canal to be ventilated. Make sure that you clean and inspect your hearing aid and ear-set as required. If an infection occurs, you should seek medical attention and contact your hearing care professional for advice on how to disinfect the various hearing aid parts. Do not under any circumstances use alcohol, chlorine or similar substances.
- Do not use Widex hearing aids in mines or other areas with explosive gases.
- **Do not wear your hearing aid during radiation, X-rays, MRIs, CT or other medical treatments and scans.** The emissions from these procedures as well as from other types of radiation, such as that in a microwave oven, can damage your hearing aid. Radiation from, for example, room surveillance equipment, burglar alarms and cell phones is weaker and will not damage the hearing aid, but may create audible interference.



## CAUTION

- Although your hearing aid has been designed to comply with the most stringent international electromagnetic compatibility standards, the possibility cannot be excluded that it may cause interference with other equipment, such as medical devices.
- Never try to open or repair the hearing aid yourself.



## ADVICE

### NOTE

- The hearing aid will not restore normal hearing and will not prevent or improve a hearing loss resulting from organic conditions. However, the hearing aid can help you to make the best possible use of your remaining hearing ability. You should also bear in mind that it can take time to get used to a new hearing aid and new sounds.
- In most cases, using the hearing aid infrequently will not permit you to gain full benefit from it.
- The use of a hearing aid is only part of hearing habilitation and may need to be supplemented by auditory training and instruction in lipreading.
- The use of hearing aids increases the risk of accumulation of earwax. Contact your physician/ENT doctor if you suspect that a plug of earwax has accumulated in your ear. Earwax may not only reduce your own hearing but also the effect of the hearing aid considerably. It is a good idea to ask your physician to clean your ears a couple of times a year.

# REGULATORY INFORMATION

## **Contraindications:**

- Congenital or traumatic deformity of the ear
- Active drainage from the ear within 90 days
- History of rapid progressive hearing loss within previous 90 days
- Acute or chronic dizziness
- Sudden unilateral hearing loss in previous 90 days

## **Important notice for prospective hearing aid users**

Good health practice requires that a person with a hearing loss have a medical evaluation by a licensed physician (preferably a physician who specializes in diseases of the ear) before purchasing a hearing aid. Licensed physicians who specialize in diseases of the ear are often referred to as otolaryngologists, otologists, or otorhinolaryngologists. The purpose of medical evaluation is to assure that all medically treatable conditions that may affect hearing are identified and treated before the hearing aid is purchased.

Following the medical evaluation, the physician will give you a written statement that states that your hearing loss has been medically evaluated and that you may be considered a candidate for a hearing aid. The physician will refer you to an audiologist or a hearing aid dispenser, as appropriate, for a hearing aid evaluation.

The audiologist or hearing aid dispenser will conduct a hearing aid evaluation to assess your ability to hear with and without a hearing aid. The hearing aid evaluation will enable the audiologist or dispenser to select and fit a hearing aid to your individual needs.

If you have reservations about your ability to adapt to amplification, you should inquire about the availability of a trial-rental or purchase-option program. Many hearing aid dispensers now offer programs that permit you to wear a hearing aid for a period of time for a nominal fee after which you may decide if you want to purchase the hearing aid.

Federal law restricts the sale of hearing aids to those individuals who have obtained a medical evaluation from a licensed physician. Federal law permits a fully informed adult to sign a waiver statement declining the medical evaluation for religious or personal beliefs that preclude consultation with a physician. The exercise of such a waiver is not in your best health interest and its use is strongly discouraged.

### **Children with hearing loss**

In addition to seeing a physician for a medical evaluation, a child with a hearing loss should be directed to an audiologist for evaluation and rehabilitation since hearing loss may cause problems in language development and the educational and social growth of a child. An audiologist is qualified by training and experience to assist in the evaluation and rehabilitation of a child with a hearing loss.




Hearing aids, accessories and batteries should not be disposed of with normal household waste. Please consult your national Widex distributor for advice on how to dispose of these items.







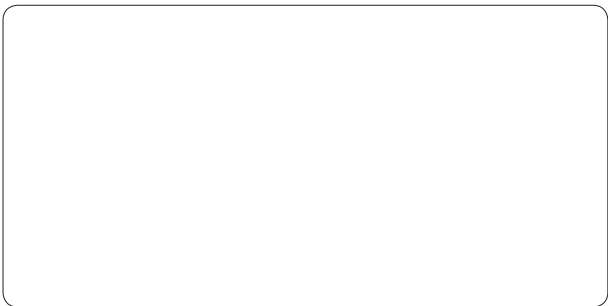

**CE** 0459

**Manufacturer**

**WIDEX A/S** • Nymoellevej 6, DK-3540 Lyngø  
Denmark • [www.widexusa.com](http://www.widexusa.com)

CIB254/0912



Printed by HTO / 2012-09  
9 514 0211 041 #02